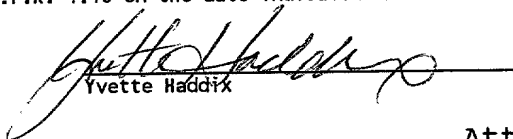


"Express Mail" Mailing Label Number: EL278352646US Date of Deposit: 5-19-99
I hereby certify that these papers are being deposited with the United States Postal Service "Express Mail Post Office to Addressee" service under 37 C.F.R. 1.10 on the date indicated above and is addressed to the Assistant Commissioner For Patents, Washington, D.C. 20231.

05/19/99
jc559 U.S. PTO


Yvette Haddix

Attorney's Docket No. MED 2 1012

UTILITY PATENT APPLICATION TRANSMITTAL LETTER
(Only for nonprovisional applications under 37 CFR 1.53(b))

jc511 U.S. PTO
09/31/99
05/19/99

Assistant Commissioner
for Patents
Washington, DC 20231-9999

Transmitted herewith for filing is a patent application of:

Schindly, et al.

for FLOW THROUGH CHEMICAL INDICATOR FOR MEASUREMENT OF ACTIVE BIOCIDAL AGENTS IN A SINGLE USE PACKAGE

Enclosed are:

[X]	<u>19</u> sheets of specification.
[X]	<u>1</u> sheet of Abstract.
[X]	<u>5</u> sheets of claims.
[X]	<u>6</u> sheets of drawings.
[X]	Assignment of an invention to <u>Steris Corp</u> .
[X]	Declaration and Power of Attorney.
[X]	PTO-1449 Form.
[]	Small Entity Statement.
[]	Certified copy of a _____ application.

CLAIMS AS FILED				
FOR	NO. FILED	NO. EXTRA	RATE	FEE
TOTAL CLAIMS	21 - 20 =	-1-	[X] \$18 LARGE	\$18.00
INDEPENDENT CLAIMS	3 - 3 =	-0-	[] \$78 LARGE	\$00.00
BASIC FEE [X] LARGE ENTITY \$760 [] SMALL ENTITY \$395.00				
TOTAL FILING FEE \$ 778.00				

____ Please charge my Deposit Account No. in the amount of \$ ____.

xx The Commissioner is hereby authorized to charge any additional filing fees which may be required for this application without specific authorization, or credit any overpayment to Deposit Account No. 06-0308.

xx Check in the amount of \$778.00 and \$40.00 to cover the filing fee and recordal fee is enclosed.

Date

May 18, 1999


Thomas E. Koeovsky, Jr.

Reg. No. 28,383

FAY, SHARPE, BEALL, FAGAN

MINNICH & MCKEE, LLP

1100 Superior Avenue, 7th Floor

Cleveland, Ohio 44114-2518

(216) 861-5582

FLOW THROUGH CHEMICAL INDICATOR FOR MEASUREMENT OF ACTIVE
BIOCIDAL AGENTS IN A SINGLE USE PACKAGE

Background of the Invention

The present invention relates to the sterilization and disinfection arts. It finds particular application in conjunction with the evaluation of the concentration of
5 peracetic acid in a sterilization or disinfection system obtained from a single use package of a concentrated decontaminant composition and will be described with particular reference thereto. It should be appreciated, however, that the invention is also applicable to other
10 liquid sterilization and disinfection processes where the sterilant or disinfectant is effective above a minimum effective concentration, such as liquid hydrogen peroxide or sodium hypochlorite sterilization or disinfection systems.

Disinfection connotes the absence of pathogenic
15 life forms. Sterilization connotes the absence of all life forms, whether pathogenic or not. The term decontamination is used herein to connote sterilization, disinfection or other antimicrobial treatments.

Until recently, medical equipment and instruments
20 were often decontaminated in a steam autoclave. Autoclaves kill life forms with a combination of high temperature and pressure. However, steam autoclaves have several drawbacks. The high temperature pressure vessels are often bulky and heavy. The high temperature and pressure tend to curtail the
25 useful life of endoscopes, rubber and plastic devices, lenses, and portions of devices made of polymeric materials and the like. Moreover, a typical autoclave decontaminating

and cool down cycle is sufficiently long that multiple sets of the medical instruments are commonly required.

Liquid decontamination systems have been developed for equipment which could not withstand the high temperatures of steam decontamination. Commonly, a technician mixes a liquid disinfectant composition immediately prior to use and manually immerses the items to be decontaminated. The high degree of manual labor introduces numerous uncontrolled and unreported variables into the process. There are quality assurance problems with the weakening of the decontaminant chemicals due to aging on the shelf, and technician errors in the mixing of decontaminant, control of immersion times, rinsing of residue, exposure to the ambient atmosphere after the rinsing step, and the like. On occasion, powdered reagents are carried away from the mixing region and deposited in undesired locations before they dissolve or react. When such systems are used for decontaminating medical instruments, undissolved reagent particles remaining on the medical instruments after a decontamination process are considered undesirable.

Recently, integrated decontamination systems, such as peracetic acid decontamination systems, have been developed which provide a premeasured dose of a decontaminant in solution. Items to be sterilized are inserted into a receiving tray of a sterilization system and a cartridge of concentrated decontaminant inserted into a well. As water flows through the system, the decontaminant is diluted and carried to the receiving tray. At the end of a decontamination cycle, the decontaminant solution is disposed of and a fresh cartridge of the concentrated decontaminant inserted into the system for the next cycle.

U.S. Patent No. 5,662,866 to Siegel, et al. discloses a two-compartment cup for use in such a system, which holds powdered sterilant reagent components. An outer cup holds a first reagent while an inner cup, disposed within the outer cup, holds a second reagent. Peripheral walls of inner and outer cups are affixed together at their open ends at flanges. A permeable sheet is affixed to the inner cup

portion flange for sealing both cups and for allowing venting of gases from the inner cup during storage. The outer cup is closed at its base by a first detachable base and the inner cup is similarly closed by a second detachable base. In use, 5 the two bases are opened to allow mixing of the two reagents. The two-compartment cup provides a reproducible, pre-measured dose of reagents, while also facilitating handling and shipping of the reagents.

It is trusted that the decontamination system will 10 be at or above the minimum effective concentration of the decontaminant for a predetermined period, so that effective decontamination is obtained. However, differences in ambient temperature, the quantity of items to be disinfected or sterilized and the level of contamination on the items can, 15 nevertheless, lead to variations in how well the decontaminant concentration is maintained over the period of the decontamination cycle. In addition, storage conditions sometimes lead to degradation of peracetic acid precursors before use. Other factors, such as poor instrument cleaning 20 or water quality may also affect decontaminant concentration. For medical instruments in particular, therefore, an additional assurance of satisfactory peracetic acid concentration is desired.

Dippable, chemically-treated papers are available 25 for checking that the peracetic acid concentration in the sterilization system reached a minimum acceptable level for sterilizing or disinfecting. A chemically-treated paper strip is typically inserted into the decontamination system and evaluated at the end of the cycle for a color change, or 30 other indication that the level of the decontaminant has been satisfactory. However, such strips are often omitted from the sterilization system, lost, or remain in the system for several cycles, and thus they are not a reliable record of whether the correct level of decontaminant was obtained in 35 each cycle.

The present invention provides for a new and improved decontaminant package and indicator system and

method of use which overcomes the above-referenced drawbacks and others.

Summary of the Invention

In accordance with one aspect of the present
5 invention, a single-use package for holding and selectively releasing a powdered composition is provided. The composition forms a solution of an anti-microbial decontaminant when mixed with water. The package includes a porous portion which is impermeable to the powdered
10 composition but is permeable to water and to the solution. An indicator on the porous portion exhibits a detectable change on exposure to the decontaminant in the solution.

In accordance with another aspect of the present invention, a package for releasing an antimicrobial
15 composition into a flowing liquid is provided. The package includes a side wall having a first opening at a first end and a second opening at a second end such that the liquid flows through the first opening into the package and out through the second opening. A layer of porous material spans
20 one of the first and second openings such that the liquid flows through the porous material layer. An antimicrobial source is disposed within the package for releasing the antimicrobial composition into the flowing liquid to form an antimicrobial solution. An indicator on the porous material
25 layer changes color in response to contact with the antimicrobial solution. The degree of color change varies in accordance with (i) the concentration of an antimicrobial agent in the solution contacting the indicator, and (ii) the duration that the solution contacts the indicator. The
30 degree of color change of the indicator is indicative of duration of contact and the concentration of the antimicrobial agent in the contacting solution.

In accordance with yet another aspect of the present invention, a method includes flowing water through a
35 cartridge containing a composition to form a decontaminant solution from the composition and the water. The cartridge includes a porous region impregnated with an indicator. The indicator exhibiting a detectable change when contacted with

a decontaminant solution for a period of time and at a concentration of a decontaminant in the solution sufficient to effect decontamination of items. The method further includes circulating the decontaminant solution in a fluid
5 flow path comprising a microbial decontamination chamber, in which the items to be decontaminated are positioned, and the porous region, and examining the indicator for the detectable change.

One advantage of the present invention is that it
10 provides a rapid method of indicating that adequate levels of a decontaminant in a decontamination cycle were maintained.

Another advantage of the present invention is that it ensures that the level of decontaminant is evaluated in every decontamination cycle.

15 Yet another advantage of the present invention is that it provides a record of decontaminant levels which may be stored with other records of the decontamination cycle.

A further advantage of the present invention is that it provides a clear yes-or-no indication of whether a
20 minimum effective concentration of peracetic acid was present during the entire cycle.

Still further advantages of the present invention will become apparent to those of ordinary skill in the art upon reading and understanding the following detailed
25 description of the preferred embodiments.

Brief Description of the Drawings

The invention may take form in various components and arrangements of components, and in various steps and arrangements of steps. The drawings are only for purposes of
30 illustrating a preferred embodiment and are not to be construed as limiting the invention.

FIGURE 1 is an exterior view of a decontamination unit according to the present invention;

FIGURE 2 is a plumbing diagram of the
35 decontamination unit of FIGURE 1 including a cross-sectional view of a reagent cartridge receiving well and one embodiment

of a two-compartment reagent package according to the present invention;

FIGURE 3 is an exploded perspective view of a first embodiment of the two compartment package in accordance with
5 the present invention;

FIGURE 4 is a side sectional view of the two-compartment package of FIGURE 3;

FIGURE 5 is an alternate embodiment of the package of FIGURES 3 and 4;

10 FIGURE 6 is a top view of a flow through top of either of the embodiments of the two compartment package of FIGURES 4 and 5 according to one embodiment of the present invention; and,

FIGURE 7A and 7B are top views of an alternate
15 embodiment of a flow through top for the two compartment packages of FIGURES 4 and 5 before (FIGURE 7A) and after (FIGURE 7B) exposure to a successful decontamination cycle.

Detailed Description of the Preferred Embodiments

20 With reference to FIGURES 1 and 2, a microbial decontamination apparatus A is configured to sit on a counter top or other convenient work surface. A door or lid 10 is manually openable to provide access to a tray 12 which defines a receiving region 14 for receiving items to be
25 microbially decontaminated. In the illustrated embodiment, the tray 12 is configured to receive endoscopes or other long, coilable items. Other trays with item receiving regions of different configurations for receiving the items themselves or item holding containers are also contemplated.
30 A well 16 receives a unit dose of reagents for forming a sterilant, disinfectant, or other microbial decontaminating solution.

With particular reference to FIGURE 2, a decontaminant containing package, cup, or cartridge C is
35 inserted into the well 16. Once the items are loaded into the tray and the decontaminant carrying cartridge C is inserted into the well 16, the lid 10 is closed and latched. A fill valve 20 passes water through a microbe removing

filter 22 in flow paths of a fluid circulating system. The
microbe removing filter 22 provides a source of sterile water
by passing water and blocking the passage of all particles
the size of microbes and larger. The incoming water which
5 has been sterilized by the filter 22 passes through a spray
or distribution nozzle 24 and fills the item receiving region
14 in the tray 12. As additional water is received, it flows
into the well 16 dissolving the decontaminant in the
cartridge C, and forming an anti-microbial solution. Filling
10 is continued until all air is forced through an air system 26
and an entire interior volume is filled with the sterile
water.

After the fill valve 20 is closed, a pump 28
circulates the fluid through a heater 30, the item receiving
15 region 14 of the tray 12, and the well 16. The pump also
forces the anti-microbial solution through the filter 22 to
a check valve 32 sterilizing the filter. Further, the pump
forces the anti-microbial solution through another microbe
filter 34 in the air system 26 to a check valve 36. After
20 the anti-microbial solution has been brought up to
temperature and circulated for a selected duration, a drain
valve 38 is opened, allowing the solution to drain. Air is
drawn through the microbe filter 34 such that sterile air
replaces the fluid within the system. Thereafter, the drain
25 valve is closed and the fill valve 20 opened again to fill
the system with a sterile rinse fluid. It will be noted,
that because the pump 28 circulated the anti-microbial
solution over all surfaces of the flow paths including all
surfaces leading from the sterile rinse source 22, the rinse
30 cannot bring microbial contaminants into the item receiving
region 14.

A lower opener projection or member 40 is
optionally disposed at the bottom of the well for engaging a
lower surface of the cartridge C as it is inserted into the
35 well, thereby opening the cartridge.

Although FIGURES 1 and 2 show a preferred
embodiment of a decontamination system A for use with a
disposable, single use cartridge C, other embodiments of the

decontamination system are also contemplated. An important feature of a suitable decontamination system is that it recirculates the decontaminant solution through the cartridge, or otherwise contacts the cartridge with the decontaminant solution, during a decontamination cycle.

With reference also to FIGURES 3-5, the single-use cartridge C contains a dose of a concentrated decontaminant for providing a decontaminant solution upon mixing with water. Specifically, the cartridge C holds a soluble decontaminant, in dry form, or two or more powdered, crystalline, or other non-liquid reagents which, when diluted with water, react to form an anti-microbial solution. The cartridge includes a porous portion 42 through which the anti-microbial solution passes during a decontamination cycle. A chemical indicator 44 for the decontaminant is printed on, or otherwise affixed to the porous portion 42 for detecting the decontaminant in the anti-microbial solution flowing through the porous portion. Since a fresh cartridge C is used with each cycle, this guarantees that a new chemical indicator is used for each cycle. Preferably, the porous portion 42 is a readily observable portion of the cartridge C, such as a lid of the cartridge, so that an operator's attention is drawn to the indicator when removing the cartridge from the decontamination system at the end of the cycle.

A variety of configurations for the decontaminant package cartridge C are contemplated. With reference to FIGURES 3 and 4, a first embodiment of the cartridge C includes a first, outer cup, or cup portion 50. The outer cup is constructed of a light weight, rigid polymeric material. The outer cup 50 includes a peripheral wall 51. The peripheral wall has a cylindrical side 52, that has a flange 54 at a first, open upper end 56 thereof, and a closure, such as a detachable base wall 58. The base wall is impermeable to a reagent disposed in the outer cup and closes a second, opposite end 60 of the side 52. The detachable base wall 58 is secured to the second end by being snapped in and held by a lip and groove, friction engagement, a

breakable seal, or the like. When force or pressure is applied to the detachable base wall from beneath the outer cup 50 by the lower opener member 40, the detachable base wall 58 detaches. An enlarged flange 62, or the like, 5 retains the base wall in the interior of the outer cup by making the diameter of the base wall larger than the opening at the second end.

A second or inner cup 70 is received in the outer cup 50. The inner cup has a generally thermally molded, 10 hemispherical peripheral wall 72 that has an integrally molded flange 74. Alternatively, the inner cup peripheral wall is cone shaped, cylindrically shaped, or the like.

With particular reference to FIGURE 4, the detachable base wall 58 has a domed central region 76. The 15 domed central region is surrounded by a vertical wall 78 that frictionally engages the cylindrical side 52 of the outer cup. As force is applied to the domed central region, it flexes. The flexing urges the attached vertical wall away from the cylindrical side of the outer cup producing the 20 frictional engagement and facilitating its release. Optionally, a plurality of legs 86 or other spaced projections are provided on the base wall for maintaining a spaced distance between the outer and inner cups upon release of the outer cup base wall 58.

25 Preferably, the inner cup peripheral wall 72 is about half the height of the outer cup peripheral wall 51 such that a first reagent chamber 88 is defined therebetween. The inner cup 70 is sealed at a first or top end 92 by a top cover 94 which provides the porous portion 42. Together, the 30 inner cup 70 and top cover 94 define a second reagent receiving chamber 96.

The peripheral wall 72 of the inner cup 70 and top cover 94 are preferably formed from a material that is impermeable to the dry reagent contained within the inner and 35 outer cups, yet is permeable to water and to dissolved reagents. Alternatively the peripheral wall 72 includes a region 98 that is formed from a material which is impermeable to powdered reagents but which is permeable to water and to

dissolved reagents. A similar region 100 is optionally included in the top cover, which defines the porous portion 42. Any particles of reagent in the inner cup 70 that are not dissolved are therefore trapped within the cartridge.

- 5 Dissolved reagents pass through the material and are transported to the items to be sterilized.

The choice of material for the top cover 94 and inner cup wall 72 depends on the particle size of the reagents. For reagents having a particle size of about 50
10 microns, a non-woven polypropylene web or felt keeps the dry reagents from penetrating the material, while allowing the water and dissolved reagents to pass freely through the inner cup 70 and top cover 94. When the material is a polypropylene web, the top cover is readily sealed to the
15 inner cup by ultrasonically welding or other heat sealing the flange of the inner cup to the top cover. Other suitable filter materials include woven polypropylene, woven or non-woven polyethylene, nylon, and rayon, rigid porous media, such as POREXTM expanded plastic, or other porous plastic,
20 fabric, felt, mesh, and analogous materials.

The material for the inner cup and top cover is preferably free of additives, such as binders or surfactants, that could be dissolved in the water and contaminate the items to be decontaminated. The material is also preferably
25 lint free, so that small particles of the material do not come away from the inner cup and become trapped within items to be decontaminated. Further, the material preferably has a fairly high tensile strength and does not disintegrate when it is subjected to a fairly high pressure of water. The
30 material is also preferably unreactive toward the reagents and other additives used in the decontamination unit. An extruded spun-bonded polypropylene web having an absolute pore size of under 50 microns, and preferably around 10 microns, is a preferred material because it is virtually
35 lint-free. It also has a high tensile strength, even when under a moderately high water pressure. The material is preferably molded to the shape of the inner cup 70 from a single sheet of the polypropylene web. Alternatively, the

flange 74 is formed from a separate material which is then welded to the remainder of the outer cup. The porous nature of the inner cup and top cover 94 allows gases formed from the reagents during transit to out gas from the cartridge C.

5 Optionally, the material also acts as a filter for filtering particles, such as microorganisms and dirt, from the anti-microbial solution passing through the cartridge.

 With continuing reference to FIGURES 3 and 4, the inner and outer cups are configured such that the flanges 54,
10 74 abut and are sealed together. Appropriate sealing means for the flanges include heat welding, adhesive bonding, solvent welding, ultrasonic welding, or the like. When the inner cup and top cover are constructed of a spun-bonded polypropylene and the outer cup is also formed from
15 polypropylene, the top cover, inner cup, and outer cups are preferably ultrasonically or heat welded together at the same time, thereby forming a seal which extends from the top cover and through the flange on the inner cup to the flange on the outer cup.

20 In an alternative version of this embodiment (not shown), the inner cup is constructed in a similar manner to the outer cup 50. Specifically, the inner cup includes a peripheral wall with a cylindrical side of slightly smaller cross sectional diameter than that of the outer cup
25 cylindrical side 52. A detachable base, similar to the outer cup base 58, closes off a lower open end of the inner cup side, while an upper open end of the inner cup side defines a flange for sealing to the outer cup flange 54. The inner cup base of this version is detached by the spaced
30 projections 86 when the outer cup base 58 is detached. A top cover 94, of the type previously described, is sealed to the inner cup flange in the manner described above.

 To assemble the cartridge C, the base 58 is first installed in the outer cup 50. The first reagent, such as a
35 dry mixture of sodium perborate, corrosion inhibitors, pH buffers, detergents and wetting agents is then disposed within the outer cup. The inner cup 70 is then placed within the outer cup with the flange 74 of the inner cup resting on

the flange 54 of the outer cup. The second reagent, preferably an acetyl donor, such as acetylsalicylic acid, is disposed within the inner cup and the top cover 94 disposed so that it rests on the flange of the inner cup. The top
5 cover, inner cup and outer cup are then sealed together at the flanges of the inner and outer cup. Specifically, the inner cup flange 74 is pressed against the outer cup flange 54 for ultrasonic or heat welding. Preferably, an outer edge of the top cover 78 is sealed to the inner cup flange 74 in
10 the same welding operation. Under heat or ultrasonic vibration, the plastic melts and flows into the fibers or into the voids of other porous filter materials, forming a unitary seal. Alternatively, other methods of sealing, such as gluing, fusion bonding, clamping with a clamping ring, or
15 the like, replace the heat or ultrasonic welding as a means of joining the various components. Thus, the first reagent is sealed within the outer cup, while the second reagent is sealed within the inner cup.

The cartridge C is configured so that substantially
20 all the water, and subsequently the decontaminant solution, entering the well 16 of the decontamination system A is forced through the top cover 94, and into contact with the indicator 44. In one preferred embodiment, the flange 54 of the outer cup is clamped into sealing contact with a rim 102
25 of the well 16 when the lid 10 of the decontamination system is closed. Alternatively, the closing of the lid brings the lower end 60 of the outer cup into sealing engagement with a base 104 of the well.

With reference to FIGURE 5, an alternate embodiment
30 of the two compartment package C' includes a first, or outer cup portion 150. The outer cup 150 is constructed of a light weight, rigid polymeric material. The outer cup 150 includes a peripheral wall 151 with a cylindrical side 152 that has a flange 154 at a first, open end 156 thereof. A fluid-
35 permeable base, or porous filter 158 covers a second, opposite, or lower end 160 of the cylindrical side 152. The porous filter 158 is ultrasonically welded or otherwise adhered to the side 152, thereby covering the lower end 160

of the outer cup. The outer cup is then filled with reagent components, such as sodium perborate, corrosion inhibitors, pH buffers, detergents and wetting agents. The filter 158 is preferably formed from a material that is impermeable to the
5 dry reagents that are contained within the outer cup portion, yet is permeable to water with dissolved reagents.

A second, or inner cup 170, similar to the inner cup 70 of the first embodiment, is received in the outer cup 150. The inner cup includes a thermally molded, peripheral
10 wall 172 which defines a generally hemispherical cup with an integrally molded flange 174. Alternatively, the inner cup peripheral wall is cone or cylindrically shaped. A first reagent-receiving chamber is 188 defined between the outer cup 150 and the inner cup peripheral wall 172. The inner cup
15 170 is filled with a second reagent component, preferably an acetyl donor such as acetylsalicylic acid.

The peripheral wall 172 of the inner cup 170 is formed, like the inner cup 70 of the first embodiment, from a filter material that is impermeable to the dry reagents
20 contained within the inner and outer cups, yet is permeable to water and to the dissolved reagents. A top opening 192 of the inner cup is covered by a top cover 194 of the same design as the top cover 94 of the first embodiment. Together the top cover 94 and the inner cup 170 define a second
25 reagent-receiving chamber 196.

In this embodiment, the porous portion 42 of the cartridge C' is provided by the top cover 194, or the fluid-permeable base 158, or both. However, because the top cover is likely to be the most visible of the two to an operator
30 when removing the cartridge after a decontamination cycle, the indicator is preferably printed on, or otherwise affixed to the top cover.

Optionally, as shown in FIGURE 5, a stiffener 202, such as an annular ring with a pair of x-shaped cross
35 members, is positioned between the inner cup 170 and the top cover 194 to ensure that the top cover lays flat. Preferably, the stiffener 202 is held in place by frictional or mechanical force.

Of course, for the embodiment of FIGURE 5, the lower opener projection 40 of the decontamination system A can be eliminated.

To assemble the cartridge C of the embodiment shown in FIGURE 5, the base 158 is first attached to the outer cup 150. The first reagent is then disposed within the outer cup. The inner cup 170 is then placed within the outer cup with the flange 74 of the inner cup resting on the flange 154 of the outer container portion. The second reagent is disposed within the inner cup and the top cover 194 disposed so that it rests on the flange of the inner cup. The top cover, inner cup and outer cup are then sealed together at the flanges of the inner and outer cups. Thus, the first reagent is sealed within the outer cup, while the second reagent is sealed within the inner cup. Other methods of assembling the cups C, C' are also contemplated.

The cartridge C is alternatively constructed according to a variety of different embodiments which serve to keep the dry reagents in separate compartments during transportation and storage, yet allow the reagents to leave the cartridge when dissolved in water, or other suitable solvent, that flows into the cartridge. Where only a single concentrated decontaminant is used, the inner compartment can, of course, be eliminated. In this case, a top cover of the type previously described is sealed directly, around a peripheral edge, to the flange 54,154 of the outer cup 50, 150.

In a preferred embodiment, the inner and outer cups 50,150,70,170 each contain one of an acid precursor and a persalt. More specifically to the preferred embodiment, the acid precursor is acetylsalicylic acid and the persalt is sodium or other perborates. The two compounds dissolve as water flows through the cartridge. The sodium perborate generates hydrogen peroxide, which, in combination with acetylsalicylic acid as an acetyl donor, forms peracetic acid.

For sterilization, the volume of powdered ingredients is selected relative to the volume of water such

that a concentration of approximately 0.2% weight/volume of peracetic acid is achieved in the resultant decontamination solution. Such a concentration is sufficient, under normal circumstances, to maintain a peracetic acid concentration of 5 at least 1500 ppm, and preferably 2000 ppm or better, throughout a sterilization cycle. For disinfection, lower concentrations of peracetic acid may be used.

The sodium perborate solution additionally functions as an inorganic corrosion inhibitor and the 10 salicylic acid as an organic corrosion inhibitor for the decontamination system and for the items to be decontaminated. Optionally, additional corrosion inhibitors, buffers, and a wetting agent are added to these powders. For hard water, in which calcium and magnesium salts may tend to 15 precipitate, a sequestering agent, such as sodium hexametaphosphate, is also included.

It is also contemplated using powdered reagents which react in a common solvent to generate chlorine gas, hydrogen peroxide, hypochlorous acid, hypochlorites, or other 20 strong oxidants which have biocidal effects.

While the cartridge has been described with reference to solid reagents, it should be appreciated that liquid reagents or decontaminants could be contained within the cartridge in addition to or in place of the dry reagents 25 by enclosing the liquid component in a sealed or leak-resistant compartment which is punctured, or otherwise opened, to release the liquid component into the decontaminant solution.

The indicator 44 is one which exhibits a detectable 30 change, such as a visible color change, when mixed with a desired concentration of the decontaminant solution. Particularly preferred are indicators which slowly change color over a period of exposure to the decontaminant solution, rather than changing color rapidly on contact with 35 the decontaminant solution. The indicator may also be temperature dependent, increasing the rate of color change with increased temperatures. Suitable indicators thus act as integrators, the final color change resulting from a

combination of the length of exposure to the decontaminant solution, the concentration of the decontaminant in the solution, and the temperature of the decontaminant solution, all of which are known to influence the effectiveness of decontamination. The color change may also be influenced by the flow rate of the decontaminant solution through the porous portion, although in most decontamination systems, the flow rate is maintained at a fairly uniform or reproducible level.

10 Absence of a color change, or only a marginal color change, indicates that the decontaminant solution was not maintained at a minimum acceptable level for decontamination, while a distinct color change indicates that a sufficient concentration was maintained for a sufficient period of time
15 to ensure sterilization or disinfection of the instruments. Optionally, the final color of the indicator after exposure to the decontaminant solution is compared with a standard color chart which identifies an acceptable color range for the level of decontamination desired.

20 Thus, when the indicator is used in a system such as the decontamination system A of FIGURES 1 and 2, the indicator does not immediately change color when it is exposed to the highly concentrated decontaminant that is initially flushed from the cartridge C. Rather, the
25 indicator progressively changes color as the decontaminant solution recirculates through the cartridge.

 The indicator is preferably one which is specific for the decontaminant and is not influenced significantly by other components of the decontaminant solution. For example,
30 in the embodiments of FIGURES 3-5, the indicator responds to peracetic acid and is not significantly influenced by the concentrations of sodium perborate, acetyl salicylic acid, hydrogen peroxide, corrosion inhibitors, buffers, wetting agents, and sequestering agents, and the like, present in the
35 decontaminant solution during a decontamination cycle. Additionally, the indicator is preferably less sensitive to pH than to the decontaminant so that it does not respond significantly to changes in pH of the decontaminant solution.

The indicator thus provides a semi-quantitative indication of the integrated level of the decontaminant in the solution over time for determining whether an acceptable level of the decontaminant was present for decontamination.

5 The indicator is preferably combined with a suitable solvent to form an ink which is printed on, or otherwise impregnated into the porous portion 42. Preferably, the ink binds to the porous material of the porous portion 42 so that the indicator is not extensively
10 leached or washed from the porous portion by the pressure of the decontaminant solution flowing through the cartridge C during the decontamination cycle. Non-woven polypropylene felts, in particular, take printing inks reasonably well and inhibit the ink from being flushed away or seeping
15 extensively throughout the porous portion.

When the decontaminant is peracetic acid to be used for sterilization of medical instruments, the indicator is preferably one which detects a concentration of between about 900 and 1800 ppm, or more of peracetic acid. The
20 concentration of peracetic acid in a sterilization system A of the type shown in FIGURE 1 naturally decreases over time so that an initial concentration of over 2000 ppm may drop to around 600-900 ppm during a sterilization cycle, depending on factors such as the level of soil on the instruments. Since
25 the indicator changes color more rapidly at higher concentrations, the overall color change will be a function of the time of exposure and the varying concentration (provided that the temperature of the system is maintained at a fairly constant level). The indicator is selected so that
30 an observable color change occurs when the peracetic acid remains at or above about 900 ppm throughout the cycle, although the indicator could be selected to trip at a different concentration level, for example, for disinfection.

Suitable indicators for peracetic acid include
35 crystal violet, bromocresol green, bromothymol blue, bromothymol green, and methyl purple, although other oxidizable indicators are also contemplated. Crystal violet is a particularly preferred indicator for peracetic acid as

it is less sensitive to changes in pH than to peracetic acid concentration. It changes color from purple to light tan or clear during a satisfactory sterilization cycle. Suitable solvents for forming an ink of the indicator include water, 5 polyvinyl alcohol, and cellulosic solvents, such as methyl cellulose, and the like. The cellulose are particularly effective for binding the ink and indicator to the porous portion 42 of the cartridge C. For crystal violet, a concentration of about 30-190 mg/l crystal violet in the ink 10 is sufficient to provide sufficient initial purple coloration and a final purple or light purple coloration in the case of an unsatisfactory cycle.

The indicator is impregnated on a central region of the top cover 94, 194, preferably during printing of labeling 15 information on the top cover. Alternatively, the indicator is soaked into the top cover and the material dried by air drying or in an oven.

Various configurations for the indicator are possible. Two preferred alternate configurations are shown 20 in FIGURES 6 and 7. In its simplest form, a region 206 of the porous portion 42 is printed or otherwise impregnated with the indicator 44. Preferably, the region 206 forms part of an upper surface 208 of the top cover 94, 194.

With reference to FIGURE 6, a region 210 of a 25 reference material is optionally also printed on the top cover 94, 194. The reference material is preferably an ink which is not affected by the decontamination process and is colored to indicate the minimum acceptable coloration of the indicator for a satisfactory decontamination cycle. The 30 reference region may be marked with the word "PASS", or other suitable indication that the color is acceptable. Optionally, a second reference region 212 is impregnated with a second ink which does not change color in the decontamination cycle. The second ink is colored to indicate 35 a coloration of the indicator after an unsatisfactory decontamination cycle, and may be marked with the word "FAIL", or similar.

With reference to FIGURES 7A and 7B, in an alternate embodiment, a region 214 of the indicator 44 is printed over the word "PASS", or similar, which is printed onto the upper surface 208 of the top cover 94 in a stable
5 ink 218. When the indicator decolorizes in a successful decontamination cycle, the word "PASS" becomes clearly visible (FIGURE 7B).

In use, the cartridge C is inserted into the well
16 of the decontamination system and items to be sterilized
10 or disinfected placed in the tray 14. Fresh water is circulated through the tray and the well. The concentrated decontaminant forms a decontaminant solution with the water which is recirculated through the tray and the well for a
15 predetermined period, contacting the indicator 44 on the porous region 42 of the top cover 94,194, or other porous region of the cartridge, in the process. The decontaminant system may then be flushed with water to remove traces of the decontaminant from the decontaminated items. The lid is
20 opened and the operator removes the spent cartridge and records the indication of decontaminant concentration provided by the indicator. If the indicator indicates that insufficient decontaminant was present in the cycle, the items are left in the tray and subjected to a second decontamination cycle with a fresh cartridge C. If the
25 indicator indicates that sufficient decontaminant was present in the cycle, the decontaminated items are removed from the system A and returned to use. The top cover 94,194 of the cartridge can be removed and stored as a permanent record for the particular cycle.

30 The invention has been described with reference to the preferred embodiment. Obviously, modifications and alterations will occur to others upon reading and understanding the preceding detailed description. It is intended that the invention be construed as including all
35 such modifications and alterations insofar as they come within the scope of the appended claims or the equivalents thereof.

Having thus described the preferred embodiment, the invention is now claimed to be:

1. A single-use package for holding a powdered composition which forms a solution of an anti-microbial decontaminant when mixed with water and for selectively releasing the composition, the package comprising:
 - 5 a porous portion which is impermeable to the powdered composition but is permeable to water and to the solution; and,
an indicator on the porous portion which exhibits a detectable change on exposure to the decontaminant in the
10 solution.
2. The package of claim 1, further including:
 - a first compartment for receiving a first component of the composition; and,
a second compartment for receiving a second
5 component of the composition, the porous portion, first compartment, and second compartment configured for forming a fluid flow path for the decontaminant solution through the package.
3. The package of claim 2, wherein the cartridge further includes:
 - an outer, first cup including a first peripheral wall with an opening at an end, the first peripheral wall
5 being at least selectively water transmissive;
an inner, second cup including a second peripheral wall, the second peripheral wall being at least selectively water transmissive, the first and second cups being configured such that the second peripheral wall abuts and is
10 connected to the first cup adjacent the end of the first peripheral wall;
 - a top cover covering the openings in the first and second cups, such that the first compartment is defined in the first cup and the second compartment is defined in the
15 second cup.

4. The package of claim 3, wherein the first peripheral wall includes a region which is formed from a first material which is impermeable to the first component but is permeable to water and to solutions containing
5 dissolved components.

5. The package of claim 3, wherein the first cup peripheral wall includes a side and a base, and wherein the base is detachable from the side.

6. The package of claim 3, wherein the second peripheral wall includes a region which is formed from a second material which is impermeable to the first and second components but is permeable to water and to solutions
5 containing dissolved components.

7. The package of claim 6, wherein the second peripheral wall defines a hemisphere and is formed from the second material.

8. The package of claim 3, wherein the top cover defines the porous portion.

9. The package of claim 1, wherein the porous portion is formed from a material selected from the group consisting of non-woven polypropylene web, woven polypropylene, woven polyethylene, non-woven polyethylene,
5 nylon, rayon, rigid porous media, porous plastic, mesh, and combinations thereof.

10. The package of claim 2, wherein the decontaminant includes peracetic acid and the first component includes acetylsalicylic acid and the second component includes sodium perborate.

11. The package of claim 1, wherein the indicator includes an oxidizable species which changes color on prolonged contact with the solution.

12. The package of claim 1 wherein the indicator is specific for the decontaminant.

13. The package of claim 1, wherein the indicator is less sensitive to pH than to the decontaminant.

14. The package of claim 1, wherein the indicator is impregnated into the porous portion in the form of an ink.

15. The package of claim 1, wherein the indicator exhibits a detectable color change when exposed to a sufficient concentration of the decontaminant for a sufficient period of time to effect decontamination.

16. The package of claim 1, wherein the decontaminant is peracetic acid and the indicator provides a detectable color change when the peracetic acid is at a concentration of about 900 ppm or above for a preselected
5 period of time.

17. The package of claim 1, wherein the decontaminant is peracetic acid and the indicator is selected from the group consisting of crystal violet, bromocresol green, bromothymol blue, bromothymol green, methyl purple,
5 and combinations thereof.

18. The package of claim 17, wherein the indicator includes crystal violet.

19. An anti-microbial system which receives the package of claim 1 comprising:

a well for receiving the package of claim 1;

5 a source of water connected with the well for mixing with the powdered composition to form the antimicrobial solution;

a microbial decontamination chamber connected with the well for receiving the anti-microbial solution, the well,
10 the porous region, and the chamber forming a recirculating fluid flow path for the decontaminant solution.

20. A package for releasing an antimicrobial composition into a flowing liquid, the package comprising:

a side wall having a first opening at a first end and a second opening at a second end such that the liquid
5 flows through the first opening into the package and out through the second opening;

a layer of porous material spanning one of the first and second openings such that the liquid flows through the porous material layer;

10 an antimicrobial source disposed within the package for releasing the antimicrobial composition into the flowing liquid to form an antimicrobial solution;

an indicator on the porous material layer which changes color in response to contact with the antimicrobial solution, a degree of color change varying in accordance with
15 (i) a concentration of an antimicrobial agent in the solution contacting the indicator, and (ii) a duration that the solution contacts the indicator such that the degree of color change of the indicator is indicative of duration of contact
20 and the concentration of the antimicrobial agent in the contacting solution.

21. A method comprising:

flowing water through a cartridge containing a composition to form a decontaminant solution from the composition and the water, the cartridge including a porous
5 region impregnated with an indicator, the indicator exhibiting a detectable change when contacted with a decontaminant solution for a period of time and at a

concentration of a decontaminant in the solution sufficient to effect decontamination of items;

- 10 circulating the decontaminant solution in a fluid flow path comprising a microbial decontamination chamber, in which the items to be decontaminated are positioned, and the porous region;

examining the indicator for the detectable change.

10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
61
62
63
64
65
66
67
68
69
70
71
72
73
74
75
76
77
78
79
80
81
82
83
84
85
86
87
88
89
90
91
92
93
94
95
96
97
98
99
100
101
102
103
104
105
106
107
108
109
110
111
112
113
114
115
116
117
118
119
120
121
122
123
124
125
126
127
128
129
130
131
132
133
134
135
136
137
138
139
140
141
142
143
144
145
146
147
148
149
150
151
152
153
154
155
156
157
158
159
160
161
162
163
164
165
166
167
168
169
170
171
172
173
174
175
176
177
178
179
180
181
182
183
184
185
186
187
188
189
190
191
192
193
194
195
196
197
198
199
200
201
202
203
204
205
206
207
208
209
210
211
212
213
214
215
216
217
218
219
220
221
222
223
224
225
226
227
228
229
230
231
232
233
234
235
236
237
238
239
240
241
242
243
244
245
246
247
248
249
250
251
252
253
254
255
256
257
258
259
260
261
262
263
264
265
266
267
268
269
270
271
272
273
274
275
276
277
278
279
280
281
282
283
284
285
286
287
288
289
290
291
292
293
294
295
296
297
298
299
300
301
302
303
304
305
306
307
308
309
310
311
312
313
314
315
316
317
318
319
320
321
322
323
324
325
326
327
328
329
330
331
332
333
334
335
336
337
338
339
340
341
342
343
344
345
346
347
348
349
350
351
352
353
354
355
356
357
358
359
360
361
362
363
364
365
366
367
368
369
370
371
372
373
374
375
376
377
378
379
380
381
382
383
384
385
386
387
388
389
390
391
392
393
394
395
396
397
398
399
400
401
402
403
404
405
406
407
408
409
410
411
412
413
414
415
416
417
418
419
420
421
422
423
424
425
426
427
428
429
430
431
432
433
434
435
436
437
438
439
440
441
442
443
444
445
446
447
448
449
450
451
452
453
454
455
456
457
458
459
460
461
462
463
464
465
466
467
468
469
470
471
472
473
474
475
476
477
478
479
480
481
482
483
484
485
486
487
488
489
490
491
492
493
494
495
496
497
498
499
500
501
502
503
504
505
506
507
508
509
510
511
512
513
514
515
516
517
518
519
520
521
522
523
524
525
526
527
528
529
530
531
532
533
534
535
536
537
538
539
540
541
542
543
544
545
546
547
548
549
550
551
552
553
554
555
556
557
558
559
560
561
562
563
564
565
566
567
568
569
570
571
572
573
574
575
576
577
578
579
580
581
582
583
584
585
586
587
588
589
590
591
592
593
594
595
596
597
598
599
600
601
602
603
604
605
606
607
608
609
610
611
612
613
614
615
616
617
618
619
620
621
622
623
624
625
626
627
628
629
630
631
632
633
634
635
636
637
638
639
640
641
642
643
644
645
646
647
648
649
650
651
652
653
654
655
656
657
658
659
660
661
662
663
664
665
666
667
668
669
670
671
672
673
674
675
676
677
678
679
680
681
682
683
684
685
686
687
688
689
690
691
692
693
694
695
696
697
698
699
700
701
702
703
704
705
706
707
708
709
710
711
712
713
714
715
716
717
718
719
720
721
722
723
724
725
726
727
728
729
730
731
732
733
734
735
736
737
738
739
740
741
742
743
744
745
746
747
748
749
750
751
752
753
754
755
756
757
758
759
760
761
762
763
764
765
766
767
768
769
770
771
772
773
774
775
776
777
778
779
780
781
782
783
784
785
786
787
788
789
790
791
792
793
794
795
796
797
798
799
800
801
802
803
804
805
806
807
808
809
810
811
812
813
814
815
816
817
818
819
820
821
822
823
824
825
826
827
828
829
830
831
832
833
834
835
836
837
838
839
840
841
842
843
844
845
846
847
848
849
850
851
852
853
854
855
856
857
858
859
860
861
862
863
864
865
866
867
868
869
870
871
872
873
874
875
876
877
878
879
880
881
882
883
884
885
886
887
888
889
890
891
892
893
894
895
896
897
898
899
900
901
902
903
904
905
906
907
908
909
910
911
912
913
914
915
916
917
918
919
920
921
922
923
924
925
926
927
928
929
930
931
932
933
934
935
936
937
938
939
940
941
942
943
944
945
946
947
948
949
950
951
952
953
954
955
956
957
958
959
960
961
962
963
964
965
966
967
968
969
970
971
972
973
974
975
976
977
978
979
980
981
982
983
984
985
986
987
988
989
990
991
992
993
994
995
996
997
998
999
1000
1001
1002
1003
1004
1005
1006
1007
1008
1009
1010
1011
1012
1013
1014
1015
1016
1017
1018
1019
1020
1021
1022
1023
1024
1025
1026
1027
1028
1029
1030
1031
1032
1033
1034
1035
1036
1037
1038
1039
1040
1041
1042
1043
1044
1045
1046
1047
1048
1049
1050
1051
1052
1053
1054
1055
1056
1057
1058
1059
1060
1061
1062
1063
1064
1065
1066
1067
1068
1069
1070
1071
1072
1073
1074
1075
1076
1077
1078
1079
1080
1081
1082
1083
1084
1085
1086
1087
1088
1089
1090
1091
1092
1093
1094
1095
1096
1097
1098
1099
1100
1101
1102
1103
1104
1105
1106
1107
1108
1109
1110
1111
1112
1113
1114
1115
1116
1117
1118
1119
1120
1121
1122
1123
1124
1125
1126
1127
1128
1129
1130
1131
1132
1133
1134
1135
1136
1137
1138
1139
1140
1141
1142
1143
1144
1145
1146
1147
1148
1149
1150
1151
1152
1153
1154
1155
1156
1157
1158
1159
1160
1161
1162
1163
1164
1165
1166
1167
1168
1169
1170
1171
1172
1173
1174
1175
1176
1177
1178
1179
1180
1181
1182
1183
1184
1185
1186
1187
1188
1189
1190
1191
1192
1193
1194
1195
1196
1197
1198
1199
1200
1201
1202
1203
1204
1205
1206
1207
1208
1209
1210
1211
1212
1213
1214
1215
1216
1217
1218
1219
1220
1221
1222
1223
1224
1225
1226
1227
1228
1229
1230
1231
1232
1233
1234
1235
1236
1237
1238
1239
1240
1241
1242
1243
1244
1245
1246
1247
1248
1249
1250
1251
1252
1253
1254
1255
1256
1257
1258
1259
1260
1261
1262
1263
1264
1265
1266
1267
1268
1269
1270
1271
1272
1273
1274
1275
1276
1277
1278
1279
1280
1281
1282
1283
1284
1285
1286
1287
1288
1289
1290
1291
1292
1293
1294
1295
1296
1297
1298
1299
1300
1301
1302
1303
1304
1305
1306
1307
1308
1309
1310
1311
1312
1313
1314
1315
1316
1317
1318
1319
1320
1321
1322
1323
1324
1325
1326
1327
1328
1329
1330
1331
1332
1333
1334
1335
1336
1337
1338
1339
1340
1341
1342
1343
1344
1345
1346
1347
1348
1349
1350
1351
1352
1353
1354
1355
1356
1357
1358
1359
1360
1361
1362
1363
1364
1365
1366
1367
1368
1369
1370
1371
1372
1373
1374
1375
1376
1377
1378
1379
1380
1381
1382
1383
1384
1385
1386
1387
1388
1389
1390
1391
1392
1393
1394
1395
1396
1397
1398
1399
1400
1401
1402
1403
1404
1405
1406
1407
1408
1409
1410
1411
1412
1413
1414
1415
1416
1417
1418
1419
1420
1421
1422
1423
1424
1425
1426
1427
1428
1429
1430
1431
1432
1433
1434
1435
1436
1437
1438
1439
1440
1441
1442
1443
1444
1445
1446
1447
1448
1449
1450
1451
1452
1453
1454
1455
1456
1457
1458
1459
1460
1461
1462
1463
1464
1465
1466
1467
1468
1469
1470
1471
1472
1473
1474
1475
1476
1477
1478
1479
1480
1481
1482
1483
1484
1485
1486
1487
1488
1489
1490
1491
1492
1493
1494
1495
1496
1497
1498
1499
1500
1501
1502
1503
1504
1505
1506
1507
1508
1509
1510
1511
1512
1513
1514
1515
1516
1517
1518
1519
1520
1521
1522
1523
1524
1525
1526
1527
1528
1529
1530
1531
1532
1533
1534
1535
1536
1537
1538
1539
1540
1541
1542
1543
1544
1545
1546
1547
1548
1549
1550
1551
1552
1553
1554
1555
1556
1557
1558
1559
1560
1561
1562
1563
1564
1565
1566
1567
1568
1569
1570
1571
1572
1573
1574
1575
1576
1577
1578
1579
1580
1581
1582
1583
1584
1585
1586
1587
1588
1589
1590
1591
1592
1593
1594
1595
1596
1597
1598
1599
1600
1601
1602
1603
1604
1605
1606
1607
1608
1609
1610
1611
1612
1613
1614
1615
1616
1617
1618
1619
1620
1621
1622
1623
1624
1625
1626
1627
1628
1629
1630
1631
1632
1633
1634
1635
1636
1637
1638
1639
1640
1641
1642
1643
1644
1645
1646
1647
1648
1649
1650
1651
1652
1653
1654
1655
1656
1657
1658
1659
1660
1661
1662
1663
1664
1665
1666
1667
1668
1669
1670
1671
1672
1673
1674
1675
1676
1677
1678
1679
1680
1681
1682
1683
1684
1685
1686
1687
1688
1689
1690
1691
1692
1693
1694
1695
1696
1697
1698
1699
1700
1701
1702
1703
1704
1705
1706
1707
1708
1709
1710
1711
1712
1713
1714
1715
1716
1717
1718
1719
1720
1721
1722
1723
1724
1725
1726
1727
1728
1729
1730
1731
1732
1733
1734
1735
1736
1737
1738
1739
1740
1741
1742
1743
1744
1745
1746
1747
1748
1749
1750
1751
1752
1753
1754
1755
1756
1757
1758
1759
1760
1761
1762
1763
1764
1765
1766
1767
1768
1769
1770
1771
1772
1773
1774
1775
1776
1777
1778
1779
1780
1781
1782
1783
1784
1785
1786
1787
1788
1789
1790
1791
1792
1793
1794
1795
1796
1797
1798
1799
1800
1801
1802
1803
1804
1805
1806
1807
1808
1809
1810
1811
1812
1813
1814
1815
1816
1817
1818
1819
1820
1821
1822
1823
1824
1825
1826
1827
1828
1829
1830
1831
1832
1833
1834
1835
1836
1837
1838
1839
1840
1841
1842
1843
1844
1845
1846
1847
1848
1849
1850
1851
1852
1853
1854
1855
1856
1857
1858
1859
1860
1861
1862
1863
1864
1865
1866
1867
1868
1869
1870
1871
1872
1873
1874
1875
1876
1877
1878
1879
1880
1881
1882
1883
1884
1885
1886
1887
1888
1889
1890
1891
1892
1893
1894
1895
1896
1897
1898
1899
1900
1901
1902
1903
1904
1905
1906
1907
1908
1909
1910
1911
1912
1913
1914
1915
1916
1917
1918
1919
1920
1921
1922
1923
1924
1925
1926
1927
1928
1929
1930
1931
1932
1933
1934
1935
1936
1937
1938
1939
1940
1941
1942
1943
1944
1945
1946
1947
1948
1949
1950
1951
1952
1953
1954
1955
1956
1957
1958
1959
1960
1961
1962
1963
1964
1965
1966
1967
1968
1969
1970
1971
1972
1973
1974
1975
1976
1977
1978
1979
1980
1981
1982
1983
1984
1985
1986
1987
1988
1989
1990
1991
1992
1993
1994
1995
1996
1997
1998
1999
2000
2001
2002
2003
2004
2005
2006
2007
2008
2009
2010
2011
2012
2013
2014
2015
2016
2017
2018
2019
2020
2021
2022
2023
2024
2025
2026
2027
2028
2029
2030
2031
2032
2033
2034
2035
2036
2037
2038
2039
2040
2041
2042
2043
2044
2045
2046
2047
2048
2049
2050
2051
2052
2053
2054
2055
2056
2057
2058
2059
2060
2061
2062
2063
2064
2065
2066
2067
2068
2069
2070
2071
2072
2073
2074
2075
2076
2077
2078
2079
2080
2081
2082
2083
2084
2085
2086
2087
2088
2089
2090
2091
2092
2093
2094
2095
2096
2097
2098
2099
2100
2101
2102
2103
2104
2105
2106
2107
2108
2109
2110
2111
2112
2113
2114
2115
2116
2117
2118
2119
2120
2121
2122
2123
2124
2125
2126
2127
2128
2129
2130
2131
2132
2133
2134
2135
2136
2137
2138
2139
2140
2141
2142
2143
2144
2145
2146
2147
2148
2149
2150
2151
2152
2153
2154
2155
2156
2157
2158
2159
2160
2161
2162
2163
2164
2165
2166
2167
2168
2169
2170
2171
2172
2173
2174
2175
2176
2177
2178
2179
2180
2181
2182
2183
2184
2185
2186
2187
2188
2189
2190
2191
2192
2193
2194
2195
2196
2197
2198
2199
2200
2201
2202
2203
2204
2205
2206
2207
2208
2209
2210
2211
2212
221

**FLOW THROUGH CHEMICAL INDICATOR FOR MEASUREMENT OF ACTIVE
BIOCIDAL AGENTS IN A SINGLE USE PACKAGE**

Abstract of the Disclosure

A single-use cartridge C contains a dose of a concentrated decontaminant for providing a decontaminant solution upon mixing with water. The cartridge is inserted into the well (16) of a decontamination system (A). Fresh water and then the decontaminant solution are recirculated through the well during a decontamination cycle. The cartridge includes a porous region (42), through which the decontaminant solution flows. Impregnated in the porous region is a chemical indicator (44), such as crystal violet, which gradually changes color on exposure to the decontaminant. The indicator provides a semi-quantitative indication of the integrated level of the decontaminant in the solution over time for determining whether an acceptable level of the decontaminant was present for decontamination.

15 A preferred embodiment of the cartridge C includes nested inner and outer water-penetrable cups (50,150,70,170) for holding first and second reagents. The two cups are sealed together adjacent upper open ends (56,92,156,192). A porous top cover (94, 194) is sealed to the inner cup adjacent the inner cup open end (92, 192) to complete the cartridge. The two reagents react with water flowing through the cartridge to form the decontaminant solution. The chemical indicator is printed on the top cover so that it is exposed to the decontaminant solution as it is recirculated through the

25 cartridge.

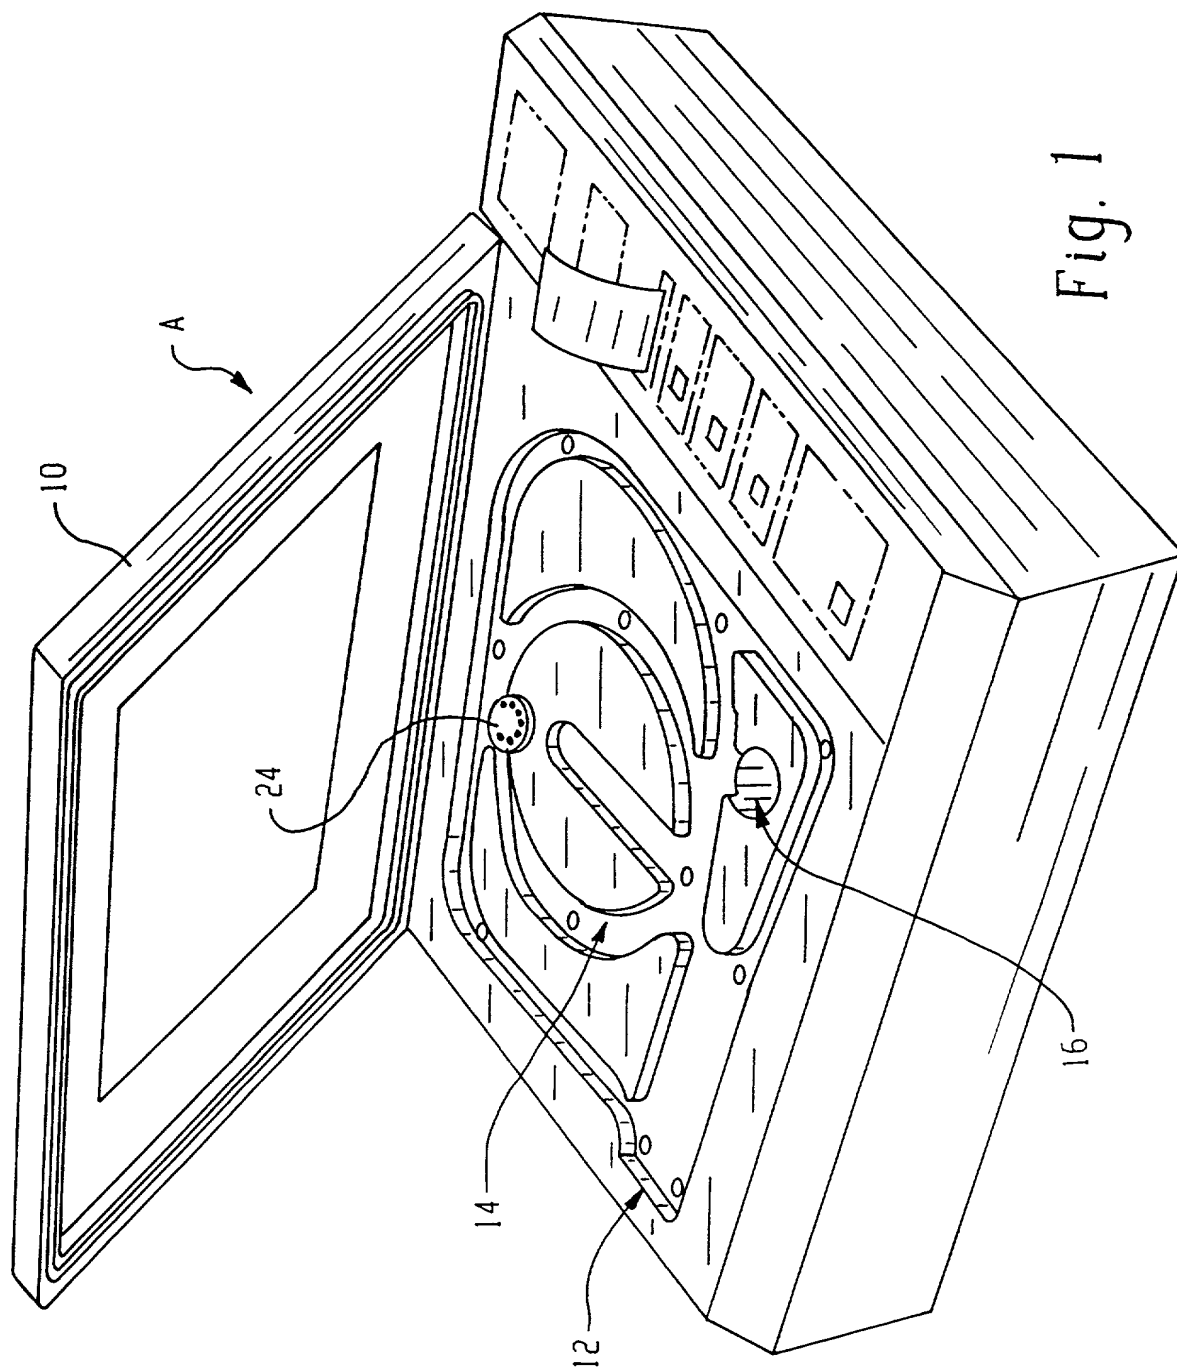
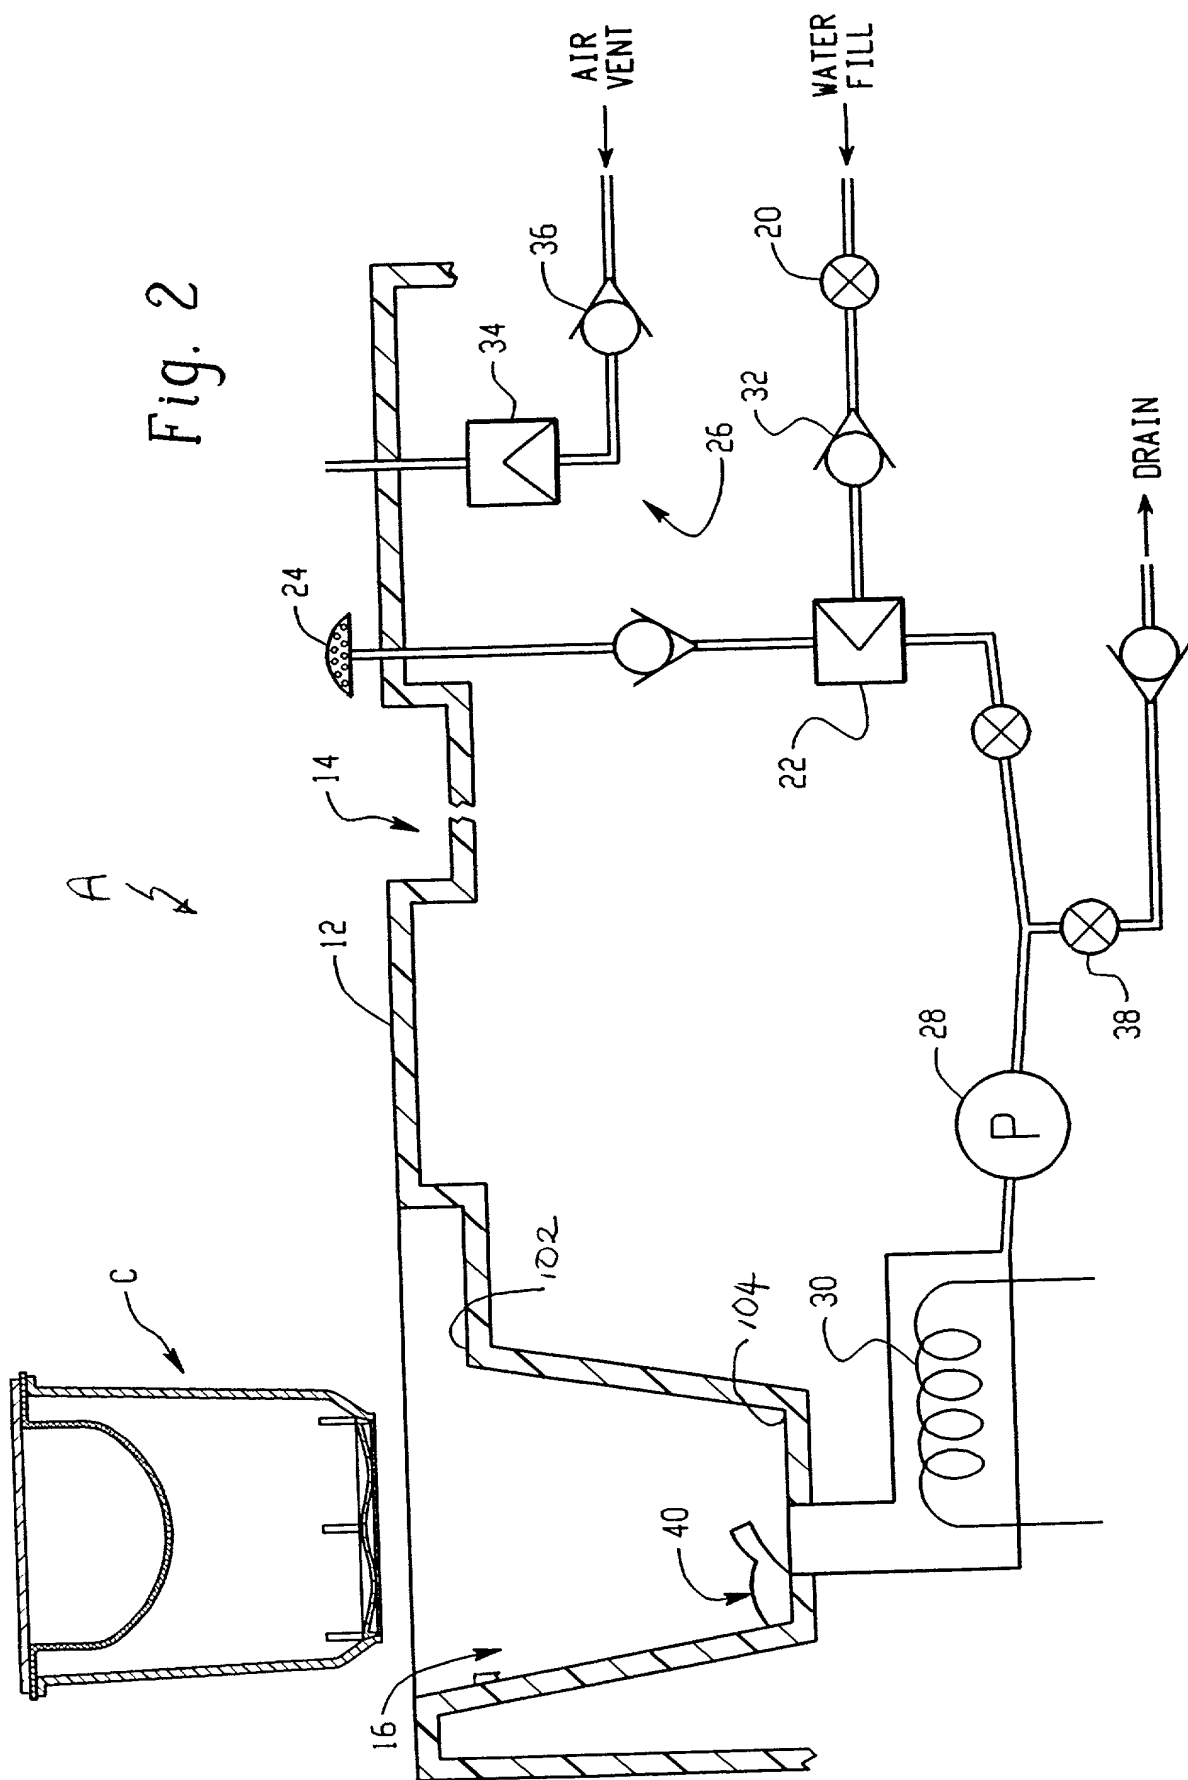


Fig. 1



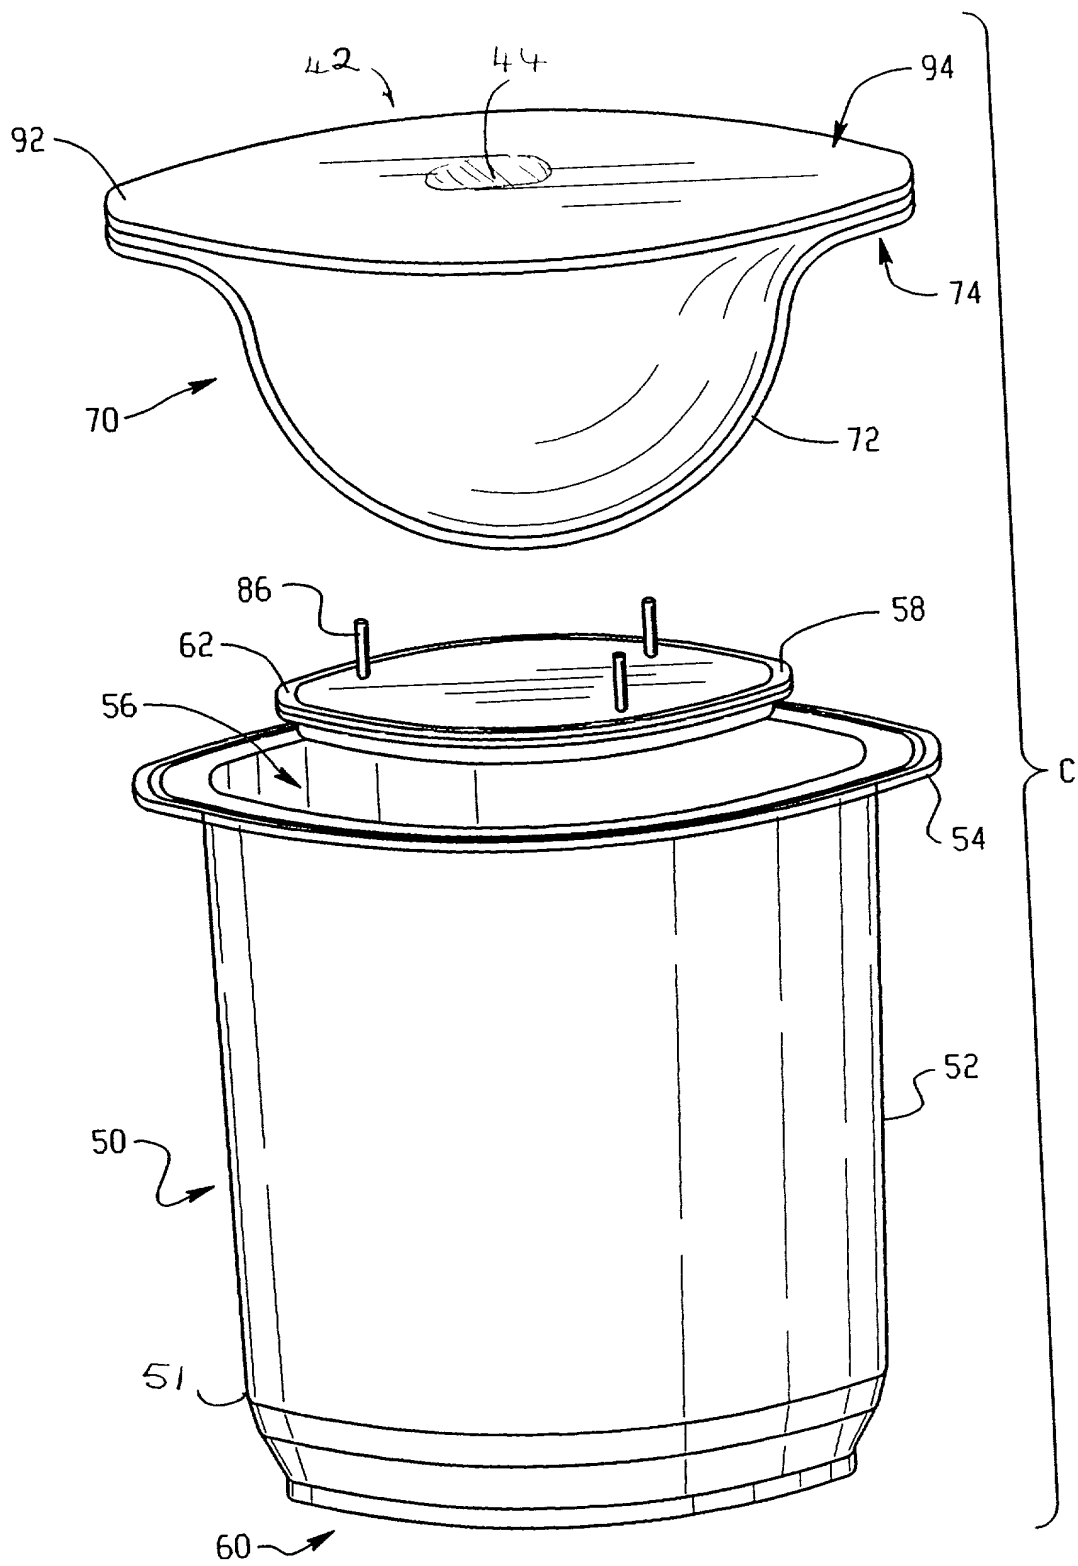


Fig. 3

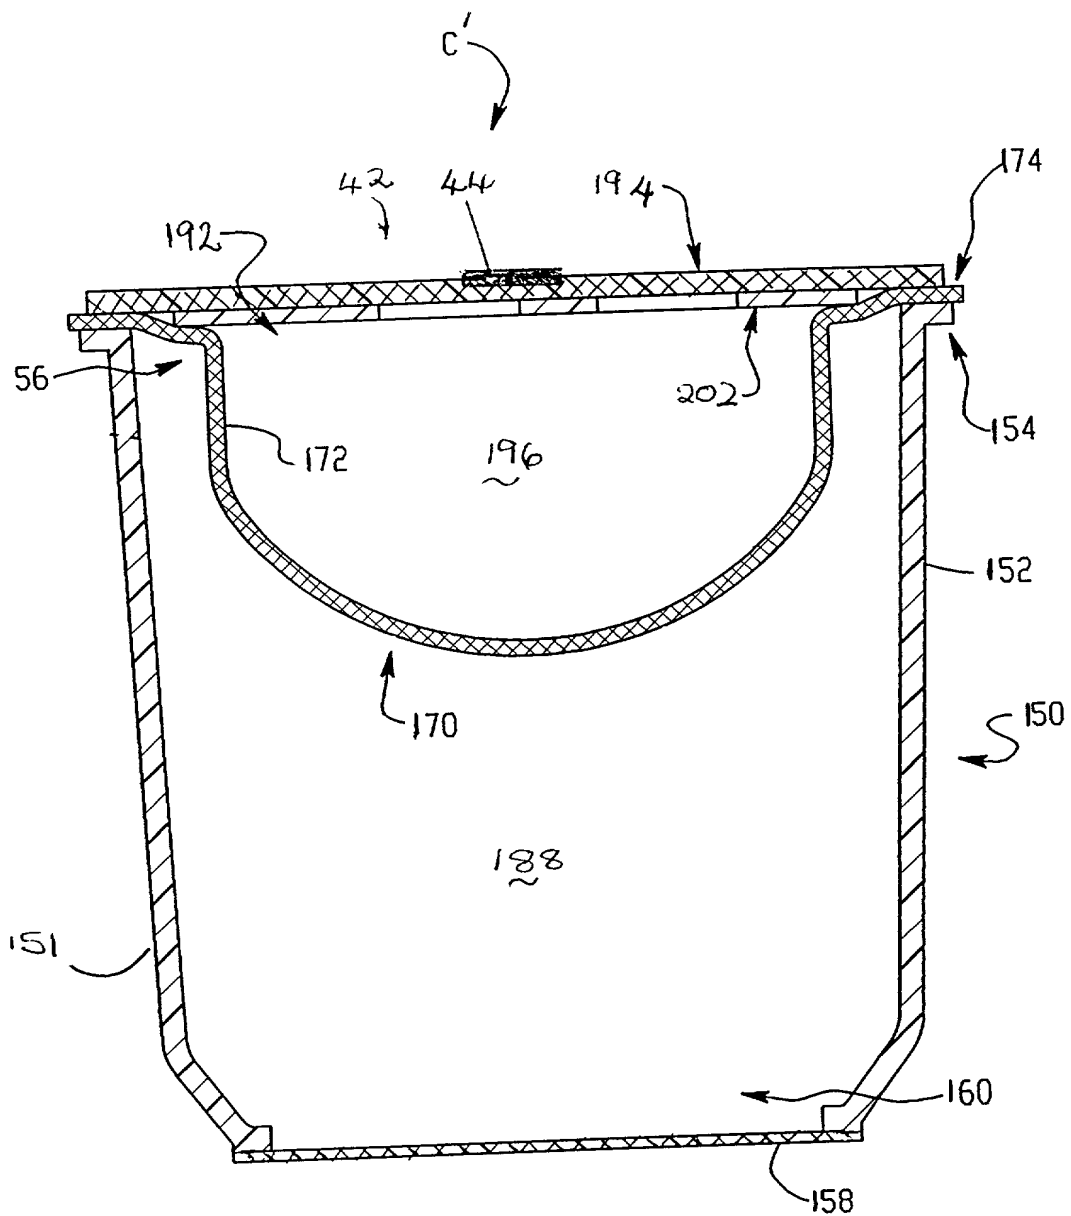


Fig. 5

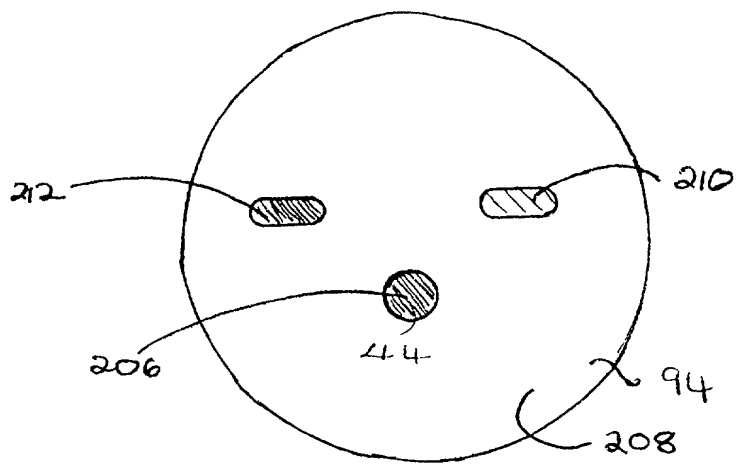


FIG. 6

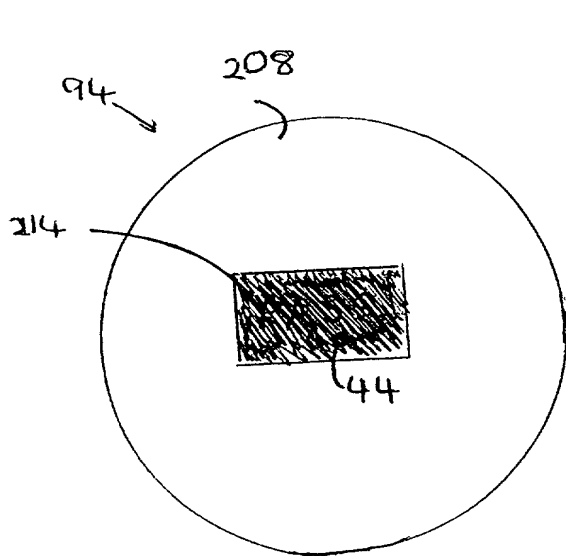


FIG. 7A

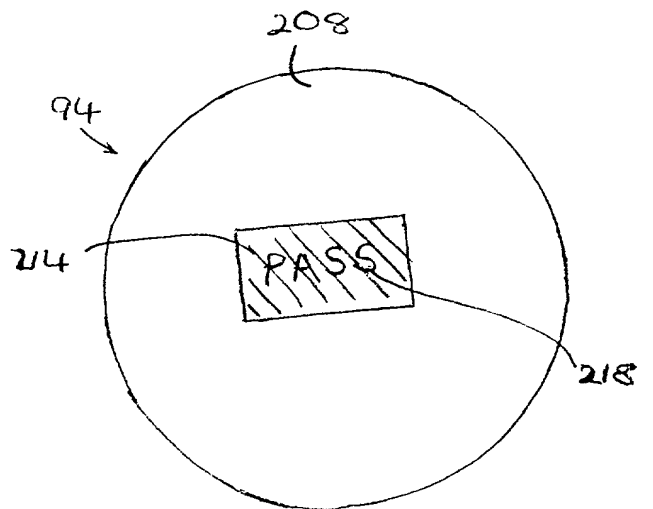


FIG. 7B

DECLARATION FOR PATENT APPLICATION

As the below named inventors, we hereby declare that:

Our residence, post office address, and citizenship are as stated below next to our names.

We believe we are an original, first, and joint inventors of the subject matter which is claimed and for which a patent is sought on the invention entitled:

**FLOW THROUGH CHEMICAL INDICATOR FOR MEASUREMENT OF ACTIVE
BIOCIDAL AGENTS IN A SINGLE USE PACKAGE**

the specification of which:

 X is attached hereto.

 has been filed and awarded Serial No. .

We hereby state that we have reviewed and understand the contents of the above-identified specification, including the claims, as amended by any amendment referred to above.

We acknowledge the duty to disclose information which is material to the examination of this application in accordance with Title 37 Code of Federal Regulations § 1.56(a).

We hereby claim foreign priority benefits under Title 35, United States Code § 119 of any foreign application(s) for patent or inventor's certificate listed below and have also identified below any foreign application for patent or inventor's certificate having a filing date before that of the application on which priority is claimed:

Not applicable

We hereby claim the benefit under Title 35, United States Code, § 119(e) of any United States provisional application(s) listed below:

Not applicable

We hereby claim the benefit under Title 35, United States Code, § 120 of any United States application(s) listed below and, insofar as the subject matter of each of the claims of this application is not disclosed in the prior United States application in the manner provided by the first paragraph of Title 35, United States Code § 112, we acknowledge the duty to disclose material information as defined in Title 37, Code of Federal Regulations, § 1.56(a) which occurred between the

filing date of the prior application and the national or PCT international filing date of this application:

Not applicable

We hereby appoint the following attorney(s) and/or agent(s) to prosecute this application and to transact all business in the Patent and Trademark Office connected therewith:

Thomas E. Kocovsky, Jr., Reg. No. 28,383
Scott A. McCollister, Reg. No. 33,961
Sandra M. Koenig, Reg. No. 33,722
Steven M. Haas, Reg. No. 37,841
John P. Cornely, Reg. No. 41,687

Address all telephone calls to: Thomas E. Kocovsky, Jr.
at telephone number: (216) 861-5582

Address all correspondence to:

Thomas E. Kocovsky, Jr.
FAY, SHARPE, BEALL, FAGAN
MINNICH & MCKEE, LLP
1100 Superior Avenue, 7th Floor
Cleveland, Ohio 44114

We hereby declare that all statements made herein of our own knowledge are true and that all statements made on information and belief are believed to be true; and further that these statements were made with the knowledge that willful false statements and the like so made are punishable by fine or imprisonment, or both, under Section 1001 of Title 18 of the United States Code and that such willful false statements may jeopardize the validity of the application or any patent issued thereon.

Full name of first joint inventor: **Brian E. Schindly**

Inventor's signature Brian E. Schindly

Date: April 22, 1999

Residence: 8404 Nowlen Street
Mentor, OH 44060
Citizenship: U.S.A.
Post Office Address: 8404 Nowlen Street
Mentor, OH 44060

Full name of second joint inventor: Christopher M. Fricker

Inventor's signature Chuph M. Fricker

Date: April 21, 1999

Residence: 7960 Fieldstone Court
Concord, OH 44060

Citizenship: U.S.A.

Post Office Address: 7960 Fieldstone Court
Concord, OH 44060

Full name of third joint inventor: George E. Grignol

Inventor's signature George E. Grignol

Date: May 6, 1999

Residence: 5401 W. 52nd Street
Fairview, Pennsylvania

Citizenship: U.S.A.

Post Office Address: 5401 W. 52nd Street
Fairview, PA 16415